



Application Guide

Sampling Train — Impingers



Impingers are specially designed bubble tubes used for collecting airborne chemicals into a liquid medium. With impinger sampling, a known volume of air is bubbled through the impinger containing a specified liquid. The liquid will chemically react with or physically dissolve the chemical of interest. This Application Guide demonstrates how to set up a **Sampling Train Using Impingers**.

Required Equipment

1. An **air sampling pump** capable of sampling at the recommended flow rate with the sampling medium in line, such as:
 - SKC Universal Series Sampler
 - SKC AirChek® 2000 Sampler
 - SKC AirChek 52 Sampler
 - SKC AirChek XR5000 Sampler
2. An **airflow calibrator**, such as:
 - Defender Primary Standard Calibrator 717 Series
3. The SKC **Impinger** specified in the method
4. **Impinger trap**, such as:
 - SKC Glass Midget Impinger Trap (without sorbent) Cat. No. 225-22
 - SKC Plastic In-line Trap (with sorbent) Cat. No. 225-22-01
5. **Impinger holder for area sampling**, such as:
 - SKC Single Glass Impinger Holder Cat. No. 225-20-01
 - SKC Double Glass Impinger Holder Cat. No. 225-20-02
 - SKC Single PFA Impinger Holder Cat. No. 225-0026
6. **Impinger holster for personal sampling**, such as:
 - SKC Glass Impinger Holster Cat. No. 225-20
 - SKC PFA Impinger Holster Cat. No. 225-0027

Optional Equipment

1. **Trap Sorbent** Cat. No. 225-22-02

Introduction

To determine the correct flow rate for the chemical of interest, refer to the appropriate analytical method. See the operating instructions for the pump to ensure that it is capable of sampling at the correct flow rate.

1. Preparing the Impinger

Fill the impinger with the recommended volume of collection liquid for sampling as specified in the analytical method.

To protect the pump from splashed or spilled impinger liquid, it is important to install a liquid trap between the impinger and the pump. Approximately one inch of solid sorbent may be added to a 225-22 trap if a volatile liquid is used in the impinger (trap 225-22-01 already contains sorbent). SKC trap sorbent will protect the pump from both organic and inorganic vapors.

2. Setting Up the Calibration Train — See Figures 1 & 2

Ensure sample pump has run for 5 minutes before calibrating the pump. Attach the stainless steel holder to the pump (Figure 1) and place the impinger and trap in the holder. With flexible tubing, connect the outlet of the impinger to the inlet (top) of the trap and the outlet (side arm) of the trap to the inlet of the pump (Figure 2).

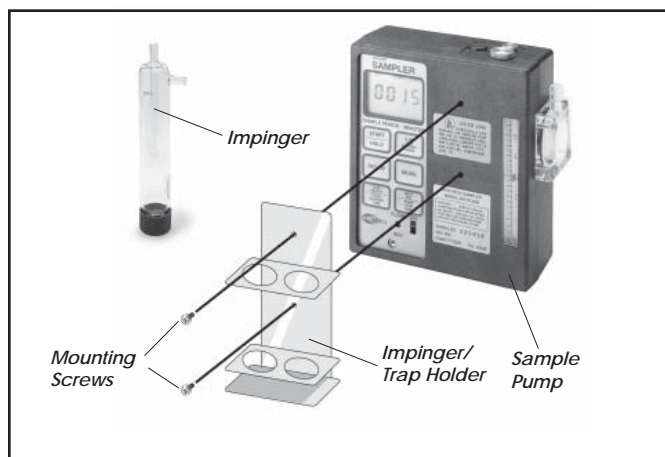


Figure 1. Attaching a glass impinger/trap holder to a sample pump

Sampling Train — Impingers

3. Calibrating the Flow Rate — See Figure 2

With flexible tubing, connect the impinger inlet to the external calibrator and calibrate to the flow rate specified in the analytical method for the chemical of interest. Typically, impinger samples are taken at 1 L/min. Refer to pump and calibrator operating instructions for calibrating the flow rate. When the flow rate has been calibrated, remove the impinger used to calibrate the flow rate. Record the pre-sample flow rate. Remove the external calibrator.

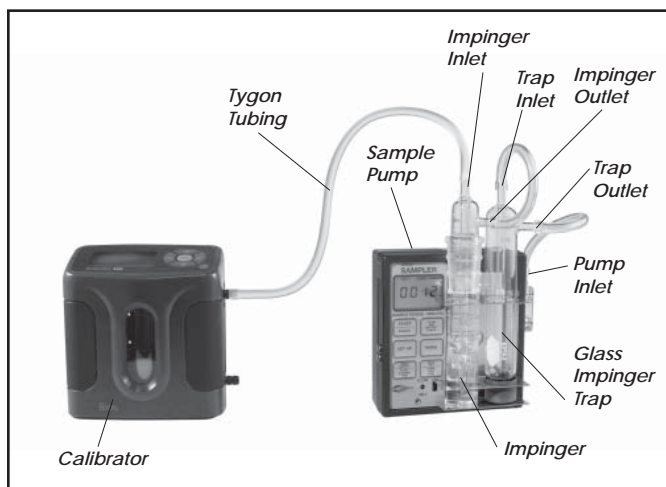


Figure 2. Glass impinger and glass trap in calibration train

4. Sampling

When ready to start sampling, prepare a new impinger with the recommended volume of collection liquid. For area sampling, place the pump with impinger and trap in the holder in the area to be sampled. For personal sampling, place the impinger in a lightweight, vinyl holster and attach it in a worker's breathing zone. Attach the pump to the worker's belt. Impinger glass and collection liquid can be a hazard when mounted on a worker; handle it carefully. Turn on the pump and note the start time and any other pertinent sampling information.

5. After Sampling

At the end of the sampling period, turn off the pump and note the ending time. Quantitatively transfer the sample solution to a glass vial. Ensure that all the solution is out of the impinger stem.

Use a calibrator and the representative impinger in line to verify that the flow has not changed by more than 5%.

Along with the sample impinger vials, submit blank samples of the impinger solution. Blank samples should be subjected to exactly the same handling as the sample except that no air is drawn through them.

Pack the samples, blanks, and all pertinent information securely for shipment to a laboratory for analysis.

6. Cleaning Impingers

Wash impingers thoroughly before reuse. Some sampling methodologies require a special preparation such as an acid wash before use.

Copyright 1996 - 2010

Notice: This publication is intended for general information only and should not be used as a substitute for reviewing applicable government regulations, equipment operating instructions, or legal standards. The information contained in this document should not be construed as legal advice or opinion nor as a final authority on legal or regulatory procedures.